

# **Amplitude Linearity Measurement and Damped Accelerometer**

---

Technical Paper 343  
By Anthony Chu

Amplitude linearity is a measure of how linear the output of an accelerometer is over its specified amplitude range. It is sometimes called amplitude non-linearity, since it specifies the deviation from perfect linearity. Manufacturers of accelerometers typically rely on several methods to measure non-linearity of the device. Here are three commonly used test apparatus and their physical characteristics:

## 1. Static Method - Centrifuge

- This is applicable only to accelerometers with DC response
- Test under static condition (one-sided loading)
- Input level is very accurate and controllable
- Max g level is only limited by the speed of the centrifuge
- Excitation frequency is at zero Hertz (static)

## 2. Sinusoidal Method - Electrodynamic shaker (suitable for only lower range devices)


- Excitation frequency is at zero Hertz (static)
- Test under dynamic condition (positive and negative loading)
- Input level is repeatable and controllable
- Max g level limited by the shaker (typically no more than 100 g)
- Excitation frequency is shaker dependent

## 3. Impulse Method - Pneumatic driven projectile (suitable for higher range devices)

- This is applicable to accelerometers with AC or DC response
- Test based on an impulse (one-sided loading)
- Input level is not well controlled
- Max g level limited by the velocity and the weight of the projectile
- Excitation frequency is dependent on the pulse width of the impact and the shape of the contact patch


With a typical accelerometer (undamped), measuring non-linearity by any of the above test methods is feasible due to the broad frequency response of an undamped design (Figure 1). In testing higher range accelerometers, impulse method is typically used due to its high acceleration capacity. However, with a damped accelerometer of higher g range ( $>100g$ ), the use of impulse method may present a practical challenge because of its inherent high frequency roll-off (Figure 2).

**Figure 1**  
Frequency response of an undamped accelerometer

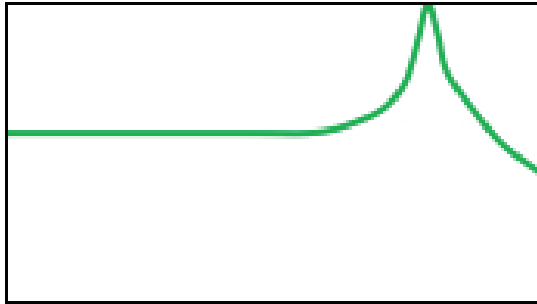

Frequency

**Figure 2**  
Frequency response of a damped accelerometer

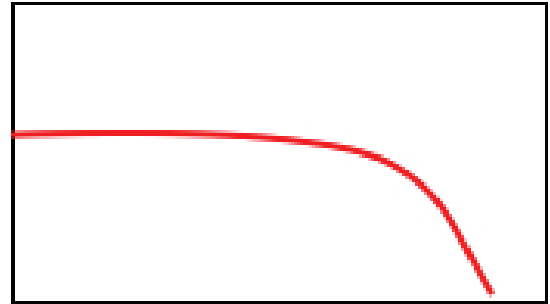


Frequency

To understand why this may be a problem in measuring non-linearity. Let's first look at the input characteristics of the impulse method. The physical construction of the impulse shock machine, typically a pneumatic driven projectile, determines the amount of energy available. The shock pulse is a function of the amplitude (g) and pulse duration (t). The maximum area under the pulse curve is fixed by the available energy of the machine. In other words, a machine can either produce higher g with short pulse duration or lower g with long pulse duration. To do both will require an impulse machine that is huge in size and complexity.


Figure 3 shows a typical input waveform created by a pneumatic driven projectile. At lower shock level ( $<1,000g$ ), the pulse width is relatively long. Its frequency spectrum can be illustrated in Figure 4.

**Figure 3**  
Time history of a lower level shock pulse

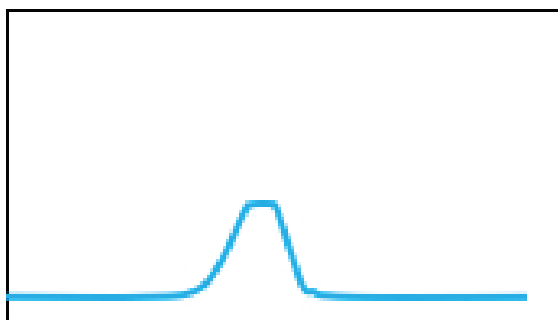


Time

**Figure 4**  
Frequency spectrum of a lower level shock pulse

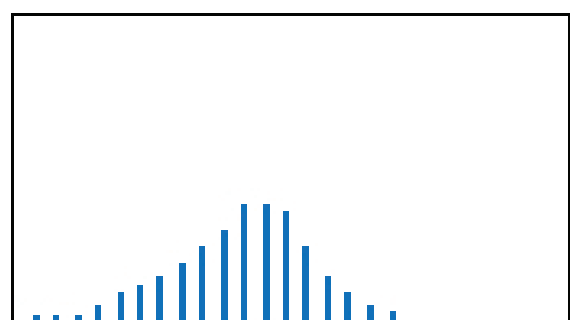

Frequency


**Figure 5**  
Bandwidth of accelerometers and input spectrum

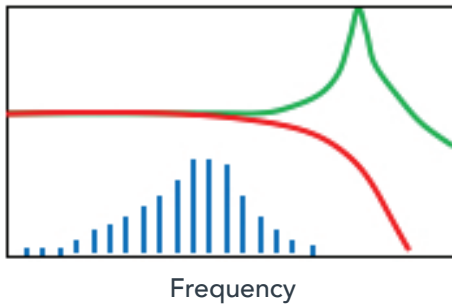


Both damped and undamped accelerometers have the necessary bandwidth to handle all the frequency components produced by such a lower level impulse, as illustrated in Figure 5.

As the shock level of the impulse shock machine increases, the pulse width gets much shorter and its rise time faster. Figure 6 and 7 show the time and frequency spectrum of a higher level shock pulse.

**Figure 6**  
Time history of a higher level shock pulse

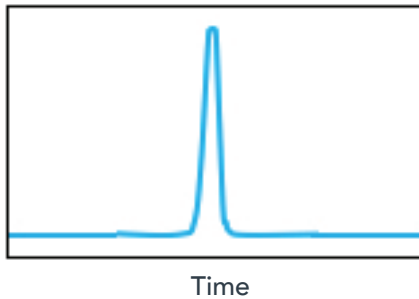


**Figure 7**  
Frequency spectrum of a higher level shock pulse

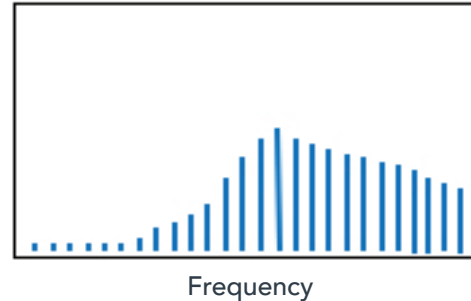

At higher g level, the shorter duration pulse contains much more high frequency components due to its fast rise time. In this case, the broad bandwidth of the undamped accelerometer still has no problem measuring the high frequency energy whereas the damped accelerometer, because of its higher frequency roll-off, is not able to capture all the higher frequency components. This is illustrated in Figure 8.

**Figure 8**  
Bandwidth of accelerometers and input spectrum

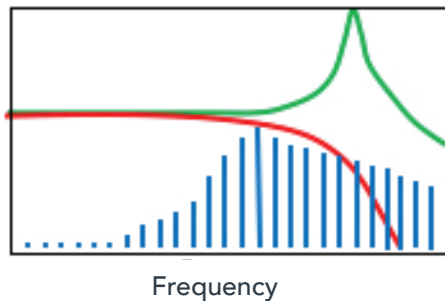

### Conclusion

When the non-linearity measurement of a damped accelerometer is conducted using an impulse method, results may suggest that the accelerometer started to get non-linear at higher g levels. However, in fact, it was due to measurement errors caused by the limited bandwidth of the accelerometer. Therefore, to accurately measure the non-linearity of a damped accelerometer, a high-g centrifuge should be used where the frequency response of the accelerometer will not be a factor in the accuracy of the measurement. The test should be conducted in both positive and negative directions in order to get a complete picture of the non linear behavior of the sensor.



[www.endevco.com](http://www.endevco.com) | Tel: +1 (866) ENDEVCO [+1 (866) 363-3826] | 10869 NC-903, Halifax, NC 27839 USA

© 2020 PCB Piezotronics of North Carolina, Inc. (doing business as Endevco). In the interest of constant product improvement, specifications are subject to change without notice. PCB®, ICP®, Swiveler®, Modally Tuned®, and IMI® with associated logo are registered trademarks of PCB Piezotronics, Inc. in the United States. ICP® is a registered trademark of PCB Piezotronics Europe GmbH in Germany and other countries. UHT-12TM is a trademark of PCB Piezotronics, Inc. SensorLine<sup>SM</sup> is a servicemark of PCB Piezotronics, Inc. MTS®, MTS Sensors logo, Temposonics®, SWIFT®, R Series V®, TempoLink®, and RefineMe® are registered trademarks of MTS Systems Corporation in the United States. These marks may be registered or otherwise protected in other countries. Endevco® is a registered trademark of PCB Piezotronics of North Carolina, Inc. d/b/a Endevco in the United States.

031620



Endevco is an assumed name of PCB Piezotronics of North Carolina, Inc. and is a designer and manufacturer of sensors, instrumentation, and cables for vibration, shock and pressure measurements, known for innovation of sensor technology for the automotive, aerospace and military markets. Visit [www.endevco.com](http://www.endevco.com) for more information. PCB Piezotronics of North Carolina, Inc. (doing business as Endevco) is a wholly owned subsidiary of PCB Piezotronics, Inc. PCB Piezotronics, Inc. is a designer and manufacturer of microphones, and vibration, pressure, force, torque, load, and strain sensors, as well as the pioneer of ICP® technology used by design engineers and predictive maintenance professionals worldwide for test, measurement, monitoring, and control requirements in automotive, aerospace, industrial, R&D, military, educational, commercial, and OEM applications. PCB also manufactures the Endevco product line of sensors, instrumentation and cables for vibration, shock and pressure measurements. With a worldwide customer support team, 24-hour SensorLine<sup>SM</sup>, and a global distribution network, PCB® is committed to Total Customer Satisfaction. Visit [www.pcb.com](http://www.pcb.com) for more information. PCB Piezotronics, Inc. is a wholly owned subsidiary of MTS Systems Corporation. Additional information on MTS can be found at [www.mts.com](http://www.mts.com).